



ANALIZA BIAŁEK



100011760

Laboratory of Analysis

Client: HEPiUS SHOP
Order number: 100011760
Name: STROMUSC MK-2866
Number of samples: 1 container

Batch number: -----
Receive date: 2026-01-02
Start date: 2026-01-23
End date: 2026-01-27

Sample identification

Substance	Method of taking a sample	Form
MK-2866	Sample provided by customer	Green tablets in a plastic container

Results

Substance	Sample name	Content	Purity
MK-2866	STROMUSC MK-2866 25MG/TAB	23,98mg/tab	-----

Research comment

The test sample was applied in the amount of 3 µl to the BioBasic 8 Thermo Scientific column. During the course of the analysis with the method a linear gradient in the solutions of H2O and Acetonitrile with the addition of 0.1% trifluoroacetic acid, a peak of the sought substance appeared. Its concentration, when compared to the reference chromatogram, is 23,98mg/tab. Height the measurement error is + - 0,05mg. The actual state of the sample sent before the test is presented on the photo below

Photo of the test sample



Password

8K3NDP94

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zająć




ANALIZA BIAŁEK



100011760

Chromatogram

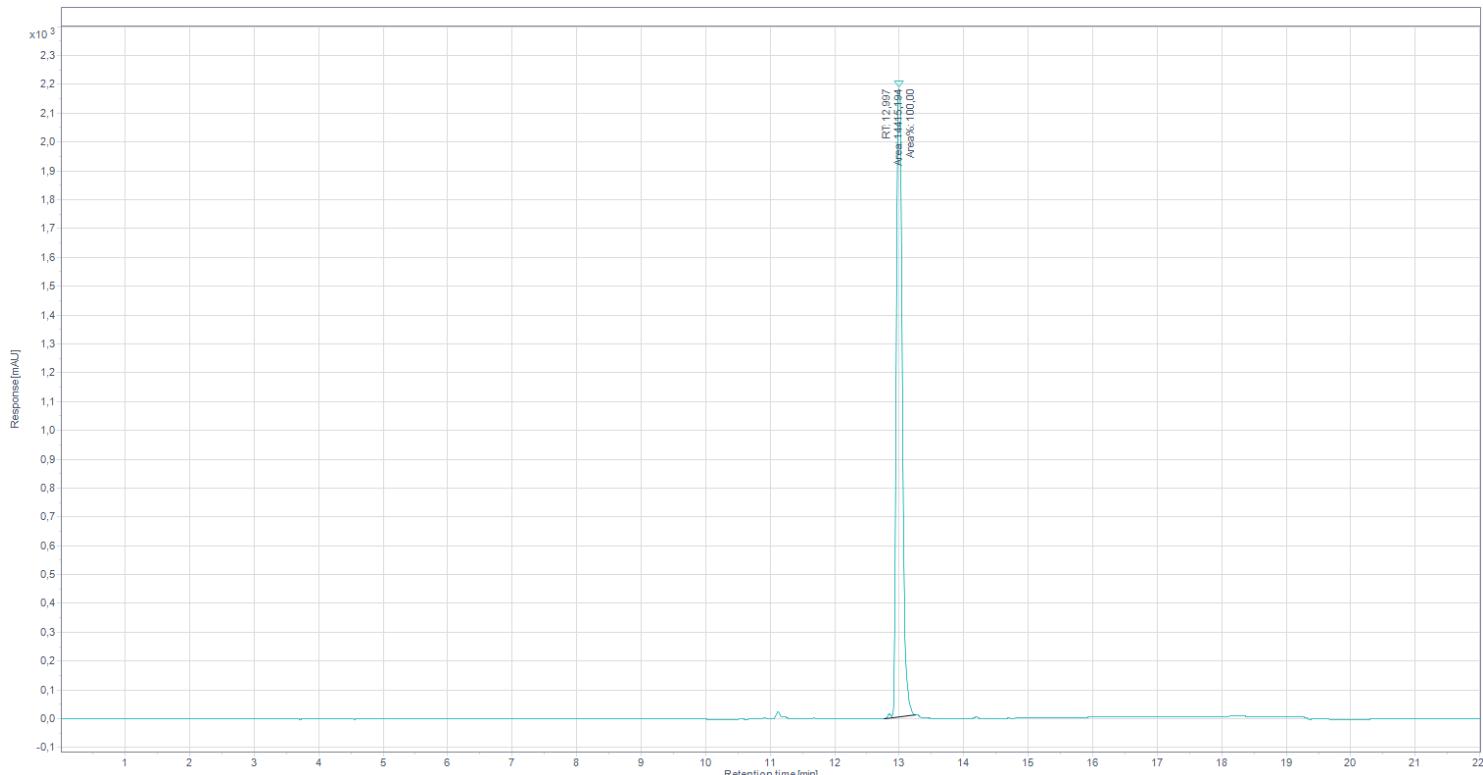

Method

Time	H ₂ O + 0,1% TFA	ACN + 0,1% TFA
0min	60%	40%
2min	60%	40%
12min	5%	95%
15min	5%	95%

Password

8K3NDP94

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac